


Danish Centre

for technical aids for rehabilitation and education
Gregersensvej - DK - 2630 Taastrup

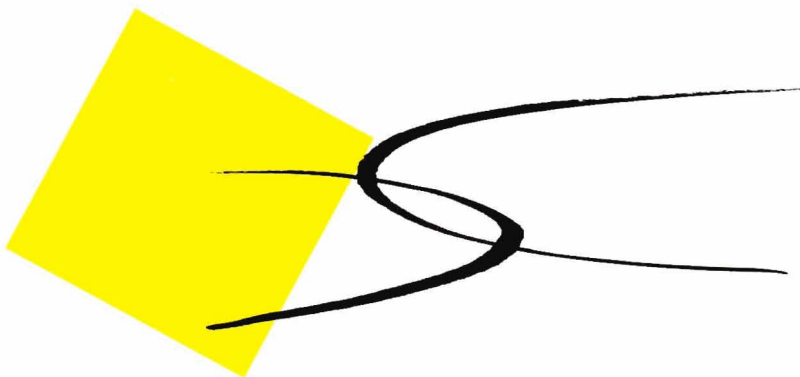

TESTING REPORT

Technical aids for disabled persons - general requirements and test methods.

according to EN 12182:1998

Testing No.
01.01

This page is page 1 of a total of 2 pages

This report should under no circumstances be reproduced, except in its total, without the permission in writing from the testing laboratory.

Notice:

This report is not an approval of the product type tested, but a record of testing results for a specific product sample

Product tested	:	Excellent System comfort module, standard
Serial no.	:	12506 12510 12503 12732 12742 12658
Product received	:	05.01.01
Testing notified by	:	Excellent System
	:	Møllevej 2
	:	DK 8544 Mørke
Person to contact	:	Ole Frederiksen
Product delivered by	:	Excellent System

03.05.2001

Date

Finn Såbye
Testing executive

Dept. of mobility, quality assurance and testing

Gregersensvej

DK- 2630 Taastrup

Tel : +45 43 99 33 22

Fax : +45 43 52 70 72

e-mail : hmi@hmi.dk

SUMMARY OF THE TESTING

A sample of type Excellent System ramp has been tested in accordance with all relevant requirements of the following sections of the EN 12182:1998 standard:

With the exception of:

- 4.2 Intended performance and technical documentation
- 17 Portable and mobile aids
- 24 Packaging

Which has not been requested.

The testing took place during the period from 05.01.2001 to 02.04.2001, and was carried out under normal indoor conditions.

If not indicated in the testing protocol, measurements were made with tolerances which can be informed from the laboratory if desired.

TESTING RESULTS

All relevant requirements of the standard were found to be fulfilled.

All relevant notes of the standard were found to be fulfilled.

The detailed testing results are recorded in the testing protocol attached.

Items marked with _____ in the protocol includes results that are not a part of the accredited testing. *It is estimated in these cases, however, that the bed/lift present no hazards when used in accordance with the manufactures instructions.*

The result in those cases are therefore based on an estimation in relation to the intended use of the product, as specified in the instructions for use.